


Supplementary

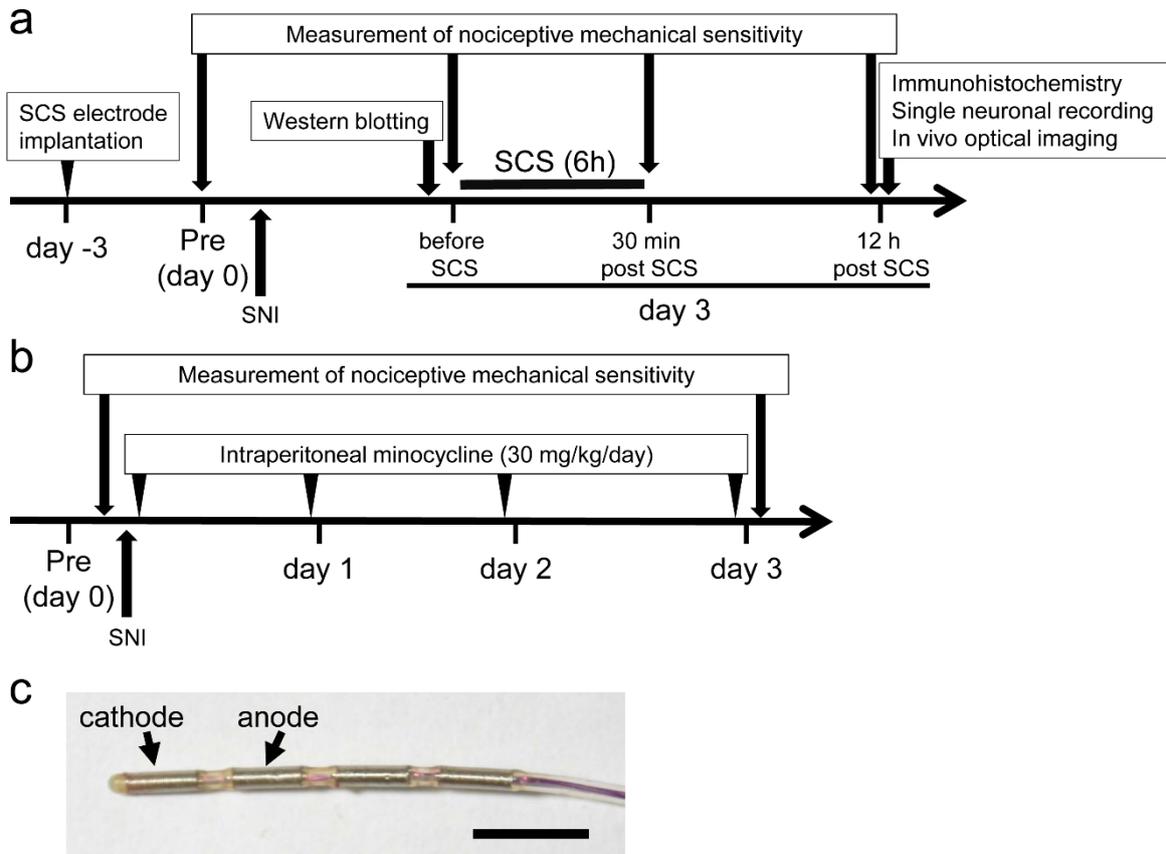

Supplementary Figure S1. Time course of each experiments. Measurement of nociceptive mechanical sensitivity of following SCS (a) or following SCS with minocycline (b). The implanted electrode (c).